

Should The Non Invasive Co2 Monitoring Be Used As A Part Of The Daily Routine?

N Akgun, G Turan, A Ozgultekin, E Dincer, C Turan, F Ormanci

Citation

N Akgun, G Turan, A Ozgultekin, E Dincer, C Turan, F Ormanci. *Should The Non Invasive Co2 Monitoring Be Used As A Part Of The Daily Routine?*. The Internet Journal of Anesthesiology. 2008 Volume 20 Number 1.

Abstract

We compared practicality and trustworthiness of invasive arterial blood gas, noninvasive ventilator monitoring, transcutaneous monitoring and pulse oxymeter on the 20 patients whom we applied mechanical ventilation in ICU. The study included 100 synchronous measures including arterial blood gas, ventilator monitor measures, transcutaneous monitor measures and patient side monitor measures of patients. No statistically significant correlation is found between ETCO_2 and PtcCO_2 as well as ETCO_2 and blood gas PCO_2 measures. A positive and good level of statistically significant correlation is found between PtcCO_2 and blood gas PCO_2 measures ($p < 0.01$). The PtcCO_2 values which were measured with transcutaneous $\text{SPO}_2/\text{PtcCO}_2$ monitor were fully correlated with blood gas CO_2 values, PtcCO_2 values are found to be superior to ETCO_2 values. When technical problems such as probe maintenance, sensor sensitivity and the need for frequent calibration are overcome, it is also considered that transcutaneous CO_2 monitoring will be an essential monitoring for ICU.

INTRODUCTION

In ICU, the continuous monitoring of CO_2 and pH of the patient who is under mechanical ventilation is as important as SPO_2 monitoring. Nowadays SPO_2 can be monitored by non invasive method in a safe and practical manner; however machines which can measure non invasive CO_2 are being tried and hence being further improved. Furthermore, same method and machine is under trial to measure pH. In our study, we compared practicality and trustworthiness of invasive arterial blood gas (PCO_2 , SatO_2), noninvasive ventilator monitoring (ETCO_2 , SPO_2 , PR), transcutaneous monitoring (PtcCO_2 , SPO_2 , PR) and pulse oxymeter (SPO_2 , PR) on the patients whom we applied mechanical ventilation in ICU.

METHODS

The study included 100 synchronous measures including arterial blood gas, ventilator monitor measures, transcutaneous monitor measures and patient side monitor measures of patients whom we applied mechanical ventilation in ICU due to various reasons. Arterial blood CO_2 pressure (PCO_2) and arterial blood O_2 saturation (SatO_2) in arterial blood gas are measured with Chiron/Diagnostic 865. End tidal CO_2 (ETCO_2), peripheral O_2 saturation [$\text{SPO}_2(\text{V})$],

peripheral pulse [$\text{PR}(\text{V})$] are measured with Drager Evita 4 (Lubeck, Germany) ventilator monitor. Transcutaneous CO_2 (PtcCO_2), peripheral O_2 saturation [$\text{SPO}_2(\text{T})$], peripheral pulse [$\text{PR}(\text{T})$] are measured with Sen Tec Digital Monitor System (V-Sign). Peripheral O_2 saturation [$\text{SPO}_2(\text{M})$] and peripheral pulse [$\text{PR}(\text{M})$] are measured with Drager Infinity Kappa (Germany) monitor saturation probe. All of these are measured and recorded synchronously and compared with each other.

Before starting the measures, the required calibration of transcutaneous monitor and ventilator is made. In all the measures, the probe of transcutaneous machine is fixed to the right ear lobe of the patient with the probe's clip. Before the measures, it's ensured that the ear lobe is clean. Difficulties such as the need for frequent calibration, re-fixation of the probe's position, and the occurrence of unexplainable errors at unexpected times are encountered. During the evaluation of the findings of the study, the SPSS for Windows 10.0 software is used for statistical analysis. During the evaluation of the data from the study, Pearson correlation analysis is used to calculate the correlation of the quantitative data along with the descriptive statistical methods (average, standard deviation). Conclusions are evaluated within the 95% confidence interval and at $p < 0.05$.

RESULTS

A positive and very good level of statistically significant correlation is found between the values of arterial blood O₂ saturation (SatO₂), peripheral O₂ saturation with ventilator monitor [SPO₂(V)], peripheral O₂ saturation with Transcutaneous monitor [SPO₂(T)], peripheral O₂ saturation with patient side monitor saturation probe. (p<0.01) (Table 1)

Figure 1

Table 1: SPO(V), SPO(M), SPO(T) ve SatO corelations

		SPO ₂ (V)	SPO ₂ (M)	SPO ₂ (T)	SatO ₂
SPO ₂ (V)	r		0,839	0,898	0,922
	p		0,001**	0,001**	0,001**
	n		100	100	100
SPO ₂ (M)	r	0,839		0,808	0,846
	p	0,001**		0,001**	0,001**
	n	100		100	100
SPO ₂ (T)	r	0,898	0,808		0,820
	p	0,001**	0,001**		0,001**
	n	100	100		100
SatO ₂	r	0,922	0,846	0,820	
	p	0,001**	0,001**	0,001**	
	n	100	100	100	

** p<0,01

A positive and very good level of statistically significant correlation is found between the measured values of ventilator monitor and peripheral pulse [PR(V)], transcutaneous monitor and peripheral pulse [PR(T)], patient side monitor probe and peripheral pulse [PR(M)] (p<0.01) (Table 2)

Figure 2

Table 2: PR(V), PR(M) ve PR(T) corelations

		PR(V)	PR(M)	PR(T)
PR(V)	r		0,993	0,988
	p		0,001**	0,001**
	n		100	100
PR (M)	r	0,993		0,989
	p	0,001**		0,001**
	n	100		100
PR (T)	r	0,988	0,989	
	p	0,001**	0,001**	
	n	100	100	

** p<0,01

No statistically significant correlation is found between ETCO₂ and PtcCO₂ as well as ETCO₂ and blood gas PCO₂ measures. (p>0.05), (Table 3).

Figure 3

Table 3: ETcO₂, PtcCO ve PCO corelations


		ETCO ₂	PtcCO ₂	PCO ₂
ETCO ₂	r		0,279	0,115
	p		0,122	0,539
	n		100	100
PtcCO ₂	r	0,279		0,677
	p	0,122		0,001**
	n	100		100
PCO ₂	r	0,115	0,677	
	p	0,539	0,001**	
	n	100	100	

** p<0,01

A positive and good level of statistically significant correlation is found between PtcCO₂ and blood gas PCO₂ measures. (p<0.01) (Graphic 1)

Figure 4

Graphic 1: PtcCO ile PCO corelation

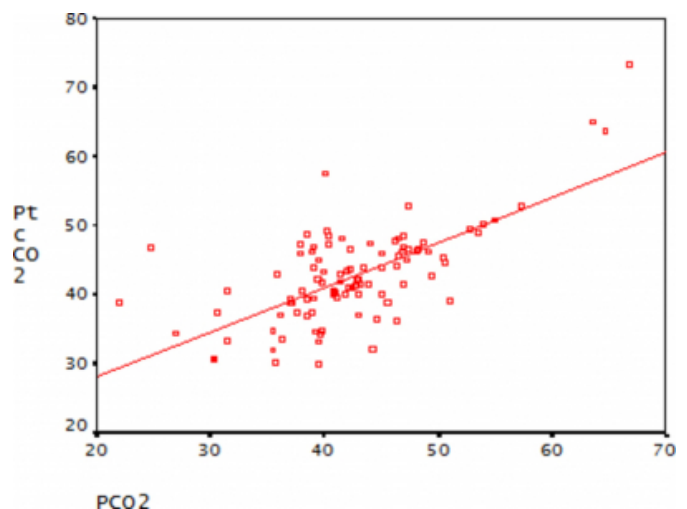

DISCUSSION

For the patients who are under mechanical ventilation in ICU as well as for the ones who are under anesthesia, the O₂ and CO₂ monitoring are the “must be performed” ones. Although monitoring with the arterial blood gas is trustable, because of the fact that it’s invasive and does not allow continuous monitoring, it is unpractical to apply. In this case, the importance of continuous noninvasive monitoring is once again highlighted. In this subject, SPO₂ monitoring

with saturation probes and ETCO_2 monitoring with gas sample taken from the expiratory branch of the ventilator circuit are the methods that have been in use for a long time. It's also a fact that ETCO_2 does not always move in parallel with the arterial CO_2 . Also our findings did not find any correlation between ETCO_2 and arterial CO_2 . Because of these reasons, search for non invasive CO_2 measure methods is continuing. In the recent years, due to ease of use, monitors tracking transcutaneous PtcCO_2 monitoring and SPO_2 through non invasive ear probe have started to be utilized (1,2,3).

McCormack et al. (2) investigated the clinical utility of transcutaneous carbon dioxide monitoring in the postoperative period, and quantified the effects of different perioperative analgesic regimens on postoperative respiratory function. They found that; the transcutaneous capnometer successfully recorded data for 98 % of the total time when it was applied to patients.

Casati A et al. (3) compared end tidal carbon dioxide (ETCO_2) with transcutaneous CO_2 measurements during mechanical ventilation in elderly patients. They reported that; transcutaneous monitoring of CO_2 partial pressure gave a more accurate estimation of arterial CO_2 partial pressure than end tidal carbon dioxide (ETCO_2) did.

Dullenkopf et al. (4) compared SPO_2 with ETCO_2 from patient side monitor and SPO_2 with PtcCO_2 from transcutaneous monitor ear probe with 111 blood gas sample taken from 60 children patients who had anesthesia. As a result, they found that transcutaneous measures were correlated with arterial blood gas and other monitor measures. They reported that transcutaneous measures can be used in anesthesia applications.

Griffin et al. (5) compared arterial blood gas PaCO_2 measures with ETCO_2 and PtcCO_2 measures in 30 morbid obese patients who had gastric bypass operation and found a better correlation between PtcCO_2 and PaCO_2 than ETCO_2 . As a result of our study, we found the same significant correlation between PtcCO_2 and PaCO_2 .

Oshibushi et al. (6) found a correlation between PtcCO_2 and ETCO_2 in 26 patients who had thorax surgery.

Nelson et al. (7) showed that they detected hypoventilation, which they could not detect prior by using only SPO_2 monitoring, by using transcutaneous SPO_2 / PtcCO_2 monitor in patients whom they applied sedation during ERCP.

Tatevossian et al. (8) utilized SPO_2 PtcCO_2 monitor during early resuscitation stage of trauma patients who had ARDS. They reported that high PtcCO_2 and low SPO_2 are important as early indicators of poor tissue perfusion in patients who died at that stage and that it can be used in daily routine.

Janssens et al. (9) found correlation between blood gas measures and monitor measures in a study in which they evaluated trustworthiness and ease of use of the transcutaneous SPO_2 / PtcCO_2 monitor. They reported that they did not have problems with the probe they fixed to the same ear for 8 hours and had no skin burns. We also did not have any skin burns during our study but we had unwanted difficulties such as no measuring or incorrect measuring. We overcame these difficulties with simple methods such as recalibration or changing the place of clip on the ear. These methods which seem simple were discouraging and time consuming.

As a conclusion of our study, as the PtcCO_2 values which were measured with transcutaneous SPO_2 / PtcCO_2 monitor were fully correlated with blood gas CO_2 values, PtcCO_2 values are found to be superior to ETCO_2 values.

Compared to blood gas monitoring, transcutaneous CO_2 monitoring is evaluated to be more comfortable for the patient and more practical for the doctor since it's non invasive and allows continuous monitoring. However the difficulties that the machine brings to users such as probe maintenance, sensor sensitivity, need for frequent calibration and need for extensive maintenance requirements in long term usage can be underestimated. It's a fact that once technical difficulties are overcome, this method will be an essential monitoring device for ICUs.

CORRESPONDENCE TO

GULDEM TURAN M.D. Barbaros M. Ihlamur S. Uphill
Court B 5 D: 2 Atasehir - Istanbul TURKEY Post Code:
34746 Tel : +900 216 4144545-1499 Fax: +900 216
3360565 E-mail: gturanmd@yahoo.com

References

1. Hinkelbein J, Floss F, Denz C, Krieter H. Accuracy and precision of three different methods to determine PCO_2 (PaCO_2 vs. PetCO_2 vs. PtcCO_2) during interhospital ground transport of critically ill and ventilated adults. J Trauma 2008; 65: 10-8.
2. McCormack JG, Kelly KP, Wedgwood J, Lyon R. The effects of different analgesic regimens on transcutaneous CO_2 after major surgery. Anaesthesia 2008; 63: 814-21.
3. Casati A, Squicciarini G, Malagutti G, Baciarello M, Putzu M, Fanelli A. Transcutaneous monitoring of partial pressure of carbon dioxide in the elderly patient: a

prospective, clinical comparison with end-tidal monitoring. J Clin Anesth. 2006; 18: 436-40.

4. Dullenkopf A, Bernardo SD, Berger F, Fasnacht M, Gerber AC, Weiss M. Evaluation of a new combined SPO2 / PtcCO2 sensor in anaesthetized paediatric patients. Paediatr Anaesth. 2003; 13: 777-84.

5. Griffin J, Terry BE, Burton RK, Ray TL, Keller BP, Landrum AL, Johnson JO, Tobias JD. Comparison of end-tidal and transcutaneous measures of carbon dioxide during general anesthesia in severely obese adults. Br J Anaesth 2003; 91: 498-501.

6. Oshibuchi M, Cho S, Hara T, Tomiyasus, Makita T, Sumikawa K. A comparative evaluation of Transcutaneous and end-tidal measurements of CO2 in thoracic anesthesia. Anesth Analg. 2003; 97: 776-9.

7. Nelson DB, Freeman ML, Silvis SE, Cass OW, Yakshe PN, Vennes J, Stahnke LL, Herman M, Hodges J. A randomized, controlled trial of transcutaneous carbon dioxide monitoring during ERCP. Gastrointestinal Endoscopy 2000; 51: 288-95.

8. Tatevossian RG, Shoemaker WC, Wo CC, Dang AB, Velmahos GC, Demetriades D. Noninvasive hemodynamic monitoring for early warning of adult respiratory distress syndrome in trauma patients. Journal of Critical Care 2000; 15: 151- 59.

9. Janssens JP, Perrin E, Bennani I, Muralt B, Titelion V, Picaud C. Is continuous transcutaneous monitoring of PCO2 (T_{cp}CO₂) over 8 h reliable in adults ? Respiratory Medicine 2001; 95: 331-35.

Author Information

Nur Akgun, M.D.

Chief, Anesthesiology and Reanimation Clinic, Fatih Sultan Mehmet Education and Research Hospital

Guldem Turan, M.D.

Consultant, II. Anesthesiology and Reanimation Clinic, Haydarpasa Numune Education and Research Hospital

Asu Ozgultekin, M.D.

Vice Chief, II. Anesthesiology and Reanimation Clinic, Haydarpasa Numune Education and Research Hospital

Emine Dincer, M.D.

Vice Chief, II. Anesthesiology and Reanimation Clinic, Haydarpasa Numune Education and Research Hospital

Cuneyt Turan, M.D.

Consultant, Anesthesiology and Reanimation Clinic, Fatih Sultan Mehmet Education and Research Hospital

Filiz Ormanci, M.D.

Consultant, II. Anesthesiology and Reanimation Clinic, Haydarpasa Numune Education and Research Hospital