

# A Review of Ankle Foot Orthotic Interventions for Patients with Stroke

M Wong, D Wong, A Wong

## Citation

M Wong, D Wong, A Wong. *A Review of Ankle Foot Orthotic Interventions for Patients with Stroke*. The Internet Journal of Rehabilitation. 2009 Volume 1 Number 1.

## Abstract

Lower limb orthotic intervention is considered as an important element in the rehabilitation of the patients with stroke. Hemiplegic gait are widely used by clinicians to describe a pattern of limb movement and body posture for the patients with stroke. This gait pattern is dangerous to the patients as it is an unstable walking pattern and has a high risk of fall. Application of ankle foot orthosis is a generally accepted method among physicians and orthotists for treating the patients with such impaired gait to prevent foot drop in swing phase. It not only facilitates toe clearance to prevent fall but also promotes heel strike in early stance. This article reviews different types of ankle foot orthoses for the rehabilitation of the patients with stroke. Such information would be useful to clinicians and researchers in selecting and developing the most appropriate ankle foot orthosis to their patients with stroke based on individual needs.

## CEREBRAL VASCULAR ACCIDENT

Cerebral Vascular Accident (CVA), also known as Stroke (International Classification of Disease 10 - ICD10: 160-169), is the third leading cause of death in Hong Kong after cancer and heart disease. More than three thousands of people died in Hon Kong each year for this condition and the proportion of total registered deaths was 8.88% [1].

Most strokes (88%) are ischemic events, including thrombosis (50%), embolism (30%), and decreased systemic perfusion (8%), while other etiologies include intracerebral hemorrhage (9%) and subarachnoid hemorrhage (3%). In 2008, the estimated direct and indirect cost of stroke was \$65.5 billion US dollars in United States of America [2].

## GAIT PATTERN OF PATIENTS WITH STROKE

Perry (1985) demonstrated that the range of ankle motion for normal subjects during walking is 10° of dorsiflexion to 15° of plantarflexion [3] but Lamontagne et al. (2002) reported that most of the patients with stroke had reduced dorsiflexion during swing phase of the affected side compared with the control values [4].


Bohannon et al. (1987 & 1991) suggested that achieving normal gait pattern and speed are usually the ultimate goal of rehabilitation for the patients with stroke. Muscle weakness, abnormal tone, sensory and visual deficits as well as decreased joint range are considered to be the important

elements that lead to affect gait speed [5, 6].

Hemiplegic gait is widely used by clinicians to describe a pattern of limb movement and body posture for the patients with stroke [7]. The patients often had inadequate shock absorption at heel strike or even worse as absence of heel strike by forefoot contact (Figure 1), inability to generate force for push off to maintain forward propulsion, and inadequate excursion of the paretic limb during swing [8, 9].

### Figure 1

Figure 1. Absence of heel strike in the initial contact for patient with stroke (adopted from Perry, 1992).

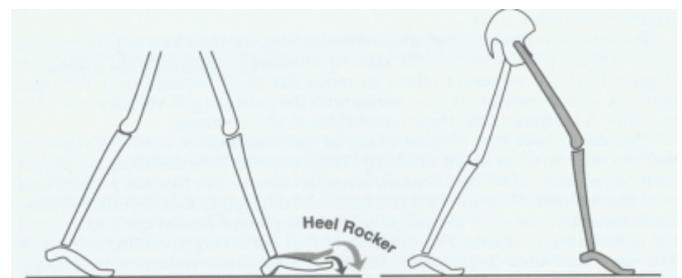

According to Olney et al. (1996), hemiplegic gait can be classified by a combination of the followings [10]:

- a reduced hip joint angle amplitude in the sagittal plane, caused by a decreased hip flexion at heel strike and a decreased hip extension at toe-off;

- a reduced knee joint angle amplitude caused by increased knee flexion at toe-off and during swing; and
- an increased plantarflexion of the ankle at heel strike & during swing, and decreased plantarflexion at toe-off.

Abnormalities of the joint kinematics often lead to secondary compensations in other body segments. The management targeted to multiple joints rather than signal joint impairment may provide more beneficial results [11]. Therefore, the evaluation of treatment should also consider the overall changes of gait pattern with multiple joints rather than those aimed at single joint.

It was suggested that evaluations of joint and segment kinematics are a valuable resource for clinical practice, since it can precisely measure the angular variations between the segments, clarify and quantify what the human eye, even with great clinical experience, is unable to do [12]. In clinical environment, gait impairments of the patients, including stride length, step length, cadence and velocity, symmetry, can be measured simply with paper walkways [13] and pressure-sensitive mat [14, 15]. The foot and gait problems can also be investigated with dynamic pressure pattern using some portable systems included in-shoe localized pressure sensor [16, 17]. A wireless system with a tri-axial accelerometer has been developed for recording the acceleration from the trunk to provide an objective measurement of walking movements as index of treatment outcome for the patients with stroke in rehabilitation [18]. Esquenazi (2002) also pointed out that the applications of joint kinematic and kinetic data provide valuable information of treatment intervention of patients with gait dysfunction [19]. Detail three-dimensional kinematic and kinetic gait profiles of persons with stroke can be identified and investigated with optoelectronic motion analysis system with force plates in laboratory environment [17, 20-24].

### **ORTHOTIC INTERVENTION FOR PATIENTS WITH STROKE**

Polypropylene Ankle Foot Orthosis (AFO) is a common choice among physicians and orthotists for treating patients with impaired gait to prevent foot drop in swing phase. It not only facilitates toe clearance but also promotes heel strike in early stance [25].

A number of studies have demonstrated the positive effect of using AFOs in the patients with stroke leading to hemiplegic

gait, but some patients are still reluctant to use rigid AFOs because of limiting ankle joint movement during ambulation. Excessive plantarflexion resistance will cause excessive knee flexion during stance phase [26, 27]. Carmick (1995) also pointed out another disadvantage of the rigid AFO was its limitation of normal movement of the tibia forwards over the weight bearing foot resulting in decreased ankle dorsiflexion and early heel rise in stance [28].

The hinged AFO with plantarflexion stop has been increasingly recommended by clinicians to prevent foot drop. An articulated AFO with planter flexion stop was found to be significantly increased the roll-over shape arc length and arc radius, and also significantly moving the sagittal plane location of the first center of pressure point posterior to the ankle center [29]. Walking with an effective roll-over may facilitate forward progression. Unlike the solid AFO, the hinged AFO allows the tibia to move forward over the weight bearing foot during stance resulting in more normal dorsiflexion motion.

Yamamoto et al. (1993) reported that the most important function of an AFO for patients with hemiplegia is to provide the dorsiflexion assisting moment, in which is normally provided by eccentric contraction of the pre-tibial muscles at the initial stance phase [30, 31]. They proposed that the plantarflexion resistive moment at the initial stance phase should be adjustable for the condition of each patient, in the range from 5 to 20 Nm per 10° of plantarflexion.

### **EFFECT OF DIFFERENT TYPES OF AFO**


Patients with hemiplegic gait are often aware of excessive backward pressure at toe off, especially going up steps and a slope, or standing up from a chair while using the conventional AFOs [32]. To decrease the excessive backward pressure, a dorsiflexion assist controlled by spring AFO (DACS-AFO) was developed by Yamamoto et al. (1991), who reported that the DACS-AFO can produce a dorsiflexion-assist moment with angle of plantarflexion at heel strike and does not refrain from dorsiflexion at toe off [33].

The Gaitsolution Orthosis (Figure 2) is another similar design from the Kawamura Gishi Co., Ltd., Japan. It targets for the patients suffering from hemiplegia after an apoplectic stroke and needing an ankle-foot orthosis for stabilisation of the ankle. Its functional design allows freedom of motion for the ankle and fast walking. Following the most recent findings [30, 31, 33-35] in the field of walking analysis, the

Gaitsolution does not stiffen the ankle joint but rather provides good motion. The heel impact on the ground is absorbed by a small hydraulic buffer inside the orthotic joint, transforming it into a flowing motion so that the patient is able to keep the balance during walking. At the same time, walking is rendered more efficient. While this method provides the stability required, the abandonment of unnecessary contact surfaces prevents a pressure feeling usually caused by an orthosis.

**Figure 2**

Figure 2. The Gaitsolution Orthosis (adopted from the Kawamura Gishi Co., Ltd.)

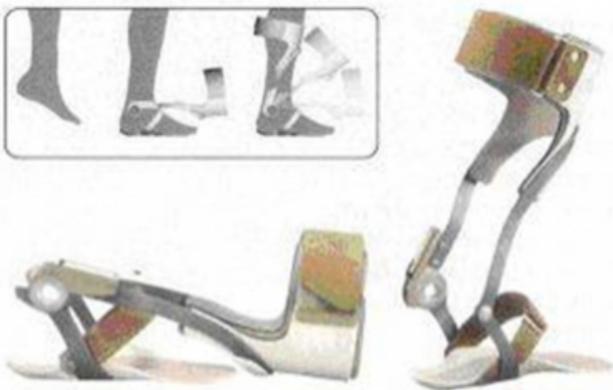

Apart from the Gaitsolution Orthosis, another design is called dream brace / joint. They were first developed by the ORTHO Incorporation, Japan. The concept of Dream Joint is to offer wider angle of plantarflexion & dorsiflexion that can get a free and smooth motion (Figures 3 & 4). A one-way frictional bearing clutch is used in the design. Unlike other mechanical joints, its dial-lock mechanism allows some ankle dorsiflexion and plantarflexion by setting the applied torque to the joint.

**Figure 3**

Figure 3. Slope walking with rigid AFO (adopted from the ORTHO Inc.)



**Figure 4**

Figure 4. Slope walking with Dream Brace (adopted from the ORTHO Inc.)



Although AFOs have been demonstrated to be beneficial to stroke gait [36], some physiotherapists still have reservation to use the orthoses. As they believed that orthoses might induce disuse effects during the period of orthotic intervention, which made the existing loss of strength getting worse and possibly delaying recovery [37]. A evaluation study was performed by Tyson's group (2001) [13] who tried to assess the effect of a hinged AFO on functional mobility and gait impairments in people with a severe hemiplegia and patients' view on the use of orthosis. Functional Ambulation Categories was used as a measure of disability. They used paper walkways to measure gait parameters and a questionnaire to determine the user's opinion of the hinged AFO. The results showed significant improvements in functional mobility and in some gait parameters.

On recent review of published literature, not many authors focus their studies on evaluation of the differences between the hinged AFOs with plantarflexion stop and the AFOs like DACS-AFO, Gaitsolution Orthosis or Dream Brace. Hachisuka et al. (1998) tried to evaluate the usefulness of DACS-AFO on five hemiplegic patients in their study [32]. Although the DACS-AFO had demonstrated excellent biomechanical characteristics, patients did not accept this AFO because of its weight, noise and appearance. The authors concluded that AFO should be further improved to make it more suitable for patients' daily usage.

Another study was performed by Yokoyama et al. (2005) [38]. They developed an AFO with oil damper unit, which provides resistance to ankle plantarflexion. They used gait analysis system to compare the kinematic effects on gait of two patients with hemiplegia at two situations - AFO with plantarflexion stop and AFO with an oil damper. The results showed that patients had sufficient plantarflexion of the ankle and mild flexion of the knee during initial stance phase

when they worn the AFOs with oil damper. The author suggested that comprehensive evaluations on kinetic, kinematic and temporal-spatial parameters of these AFO were required.

Yamamoto et al. (2005) performed a study on AFO with an oil damper – the GaitSolution Orthosis [34]. They tried to investigate the effect of this AFO on gait of three patients with hemiplegia by three-dimensional motion analysis system. It was found that the adequate resistive moment of the GaitSolution Orthosis would help to compensate for insufficient activity of the dorsiflexors. The rigid AFO with plantarflexion stop causing the shank moved forward excessively and rapidly at the time from heel strike to foot flat. This resulted in instability of knee joint. By the use of the GaitSolution Orthosis, gait pattern with minimized hyperextension or instability of the knee joint and smooth progression of the body during stance phase were noted. The authors concluded that the GaitSolution Orthosis is a useful device for gait training because it prevents rapid plantar flexion but allows gradual plantarflexion in stance phase. Subjective information of the comfortability of the patients in using the GaitSolution Orthosis was also evaluated with a questionnaire. It was reported that patients felt comfortable in using GaitSolution Orthosis mainly depending on trunk posture and hip joint outward rotation especially in the recovery phase [35].

### CONCLUSION

This article reviews different types of ankle foot orthoses for preventing drop foot gait of the patients with stroke. These orthoses included rigid, semi-rigid, plantar flexion resist and dorsiflexion assist types. The selection of orthosis should be based on the physical condition, activity level and living environment of the patients. A more appropriate ankle foot orthosis could allow the patients with stroke to better adapt to their daily activities and reintegration to the society.

### References

1. Hong Kong Hospital Authority, 2005/06. Hospital Authority Statistical Report.
2. American Heart Association, 2008. Heart Disease and Stroke Statistics.
3. Perry, J., 1985. Normal and pathological gait. Series, St. Louis, Mo: C.V. Mosby Co.
4. Lamontagne, A., Malouin, F., Richards, C. L. and Dumas, F., 2002. Mechanisms of disturbed motor control in ankle weakness during gait after stroke. *Gait Posture*, 15 (3), 244-255.
5. Bohannon, R. W., Horton, M. G. and Wikholm, J. B., 1991. Importance of four variables of walking to patients with stroke. *Int J Rehabil Res*, 14 (3), 246-250.
6. Bohannon, R. W., Larkin, P. A., Smith, M. B. and Horton, M. G., 1987. Relationship between static muscle strength deficits and spasticity in stroke patients with hemiparesis. *Phys Ther*, 67 (7), 1068-1071.
7. Kuan, T. S., Tsou, J. Y. and Su, F. C., 1999. Hemiplegic gait of stroke patients: the effect of using a cane. *Arch Phys Med Rehabil*, 80 (7), 777-784.
8. Perry, J., 1992. *Gait Analysis: Normal and Pathological Function*. Series, SLACK Incorporated.
9. Chen, G., Patten, C., Kothari, D. H. and Zajac, F. E., 2005. Gait differences between individuals with post-stroke hemiparesis and non-disabled controls at matched speeds. *Gait Posture*, 22 (1), 51-56.
10. Olney, S. and Richards, C., 1996. Hemiplegic gait following stroke. Part I: Characteristic. *Gait Posture*, 4 136-148.
11. Cruz, T. H., Lewek, M. D. and Dhaher, Y. Y., 2009. Biomechanical impairments and gait adaptations post-stroke: multi-factorial associations. *J Biomech*, 42 (11), 1673-1677.
12. Lucareli, P. R. and Greve, J. M., 2006. Alteration of the load-response mechanism of the knee joint during hemiparetic gait following stroke analyzed by 3-dimensional kinematic. *Clinics (Sao Paulo)*, 61 (4), 295-300.
13. Tyson, S. F. and Thornton, H. A., 2001. The effect of a hinged ankle foot orthosis on hemiplegic gait: objective measures and users' opinions. *Clin Rehabil*, 15 (1), 53-58.
14. Patterson, K. K., Gage, W. H., Brooks, D., Black, S. E. and McIlroy, W. E., 2009. Evaluation of gait symmetry after stroke: A comparison of current methods and recommendations for standardization. *Gait Posture*, 15. Patterson, K. K., Parafianowicz, I., Danells, C. J., Closson, V., Verrier, M. C., Staines, W. R., Black, S. E. and McIlroy, W. E., 2008. Gait asymmetry in community-ambulating stroke survivors. *Arch Phys Med Rehabil*, 89 (2), 304-310.
16. Barton, J. G. and Lees, A., 1995. Development of a connectionist expert system to identify foot problems based on under-foot pressure patterns. *Clin Biomech (Bristol, Avon)*, 10 (7), 385-391.
17. Wong, A. M., Pei, Y. C., Hong, W. H., Chung, C. Y., Lau, Y. C. and Chen, C. P., 2004. Foot contact pattern analysis in hemiplegic stroke patients: an implication for neurologic status determination. *Arch Phys Med Rehabil*, 85 (10), 1625-1630.
18. Mizuike, C., Ohgi, S. and Morita, S., 2009. Analysis of stroke patient walking dynamics using a tri-axial accelerometer. *Gait Posture*, 30 (1), 60-64.
19. Esquenazi, A., 2002. Clinical application of joint kinetic analysis in gait. *Phys med and Rehab*, 16 (2), 201-213.
20. Bleyenheuft, C., Caty, G., Lejeune, T. and Detrembleur, C., 2008. Assessment of the Chignon dynamic ankle-foot orthosis using instrumented gait analysis in hemiparetic adults. *Ann Readapt Med Phys*, 51 (3), 154-160.
21. Cruz, T. H. and Dhaher, Y. Y., 2009. Impact of ankle-foot-orthosis on frontal plane behaviors post-stroke. *Gait Posture*, 30 (3), 312-316.
22. Gok, H., Kucukdeveci, A., Altinkaynak, H., Yavuzer, G. and Ergin, S., 2003. Effects of ankle-foot orthoses on hemiparetic gait. *Clin Rehabil*, 17 (2), 137-139.
23. Kaczmarczyk, K., Wit, A., Krawczyk, M. and Zaborski, J., 2009. Gait classification in post-stroke patients using artificial neural networks. *Gait Posture*, 30 (2), 207-210.
24. Kim, C. M. and Eng, J. J., 2004. Magnitude and pattern of 3D kinematic and kinetic gait profiles in persons with stroke: relationship to walking speed. *Gait Posture*, 20 (2), 140-146.
25. Leung, J. and Moseley, A., 2003. Impact of ankle-foot orthoses on gait and leg muscle activity in adults with hemiplegia: systematic literature review. *Phys Ther*, 89

39-55.

26. Lehmann, J. F., Condon, S. M., Price, R. and deLateur, B. J., 1987. Gait abnormalities in hemiplegia: their correction by ankle-foot orthoses. *Arch Phys Med Rehabil*, 68 (11), 763-771.

27. Lehmann, J. F., Esselman, P. C., Ko, M. J., Smith, J. C., deLateur, B. J. and Dralle, A. J., 1983. Plastic ankle-foot orthoses: evaluation of function. *Arch Phys Med Rehabil*, 64 (9), 402-407.

28. Carmick, J., 1995. Managing equinus in a child with cerebral palsy: merits of hinged ankle-foot orthoses. *Dev Med Child Neurol*, 37 (11), 1006-1010.

29. Fatone, S. and Hansen, A. H., 2007. Effect of ankle-foot orthosis on roll-over shape in adults with hemiplegia. *J Rehabil Res Dev*, 44 (1), 11-20.

30. Yamamoto, S., Ebina, M., Iwasaki, M., Kubo, S., Kawai, H. and Kayashi, T., 1993. Comparative study of mechanical characteristics of plastic AFOs. *JPO*, 5 (2), 59-67.

31. Yamamoto, S., Ebina, M., Kubo, S., Kawai, H., Hayashi, T., Iwasaki, M., Kubota, T. and Miyazaki, S., 1993.

Quantification of the effect of dorsi-/plantarflexibility of ankle foot orthoses on hemiplegic gait: A preliminary report. *JPO* 5(2), 88-95.

32. Hachisuka, K., Ogata, H., Tajima, F. and Ohmine, S., 1998. Clinical evaluations of dorsiflexion assist controlled

by spring ankle-foot orthosis for hemiplegic patients. *J Uoeh*, 20 (1), 1-9.

33. Yamamoto, S., Ebina, M., Kubo, S., Dohi, T. and Hayakawa, Y., 1991. Development of dorsiflexion assist controlled by spring ankle-foot orthosis (DACs AFO) for hemiplegic patients. *Proceeding of 15th Biomechanism Symposium*, 301-309.

34. Yamamoto, S., Hagiwara, A., Mizobe, T. and Yokoyama, O., 2005. Development of an ankle-foot orthosis with an oil damper. *JPO* 29 (3), 209-219.

35. Yamamoto, S., Hagiwara, A., Mizobe, T., Yokoyama, O. and Yasui, T., 2009. Gait improvement of hemiplegic patients using an ankle-foot orthosis with assistance of heel rocker function. *Prosthet Orthot Int*, 33 (4), 307-323.

36. Jaiwin, J. S., Bishop, J. O., Braly, W. G. and Tullos, H. S., 1992. Management of acquired adult dropfoot. *Foot Ankle*, 13 (2), 98-104.

37. Appell, H. J., 1990. Muscular atrophy following immobilisation. A review. *Sports Med*, 10 (1), 42-58.

38. Yokoyama, O., Sashika, H., Hagiwara, A., Yamamoto, S. and Yasui, T., 2005. Kinematic effects on gait of a newly designed ankle-foot orthosis with oil damper resistance: a case series of 2 patients with hemiplegia. *Arch Phys Med Rehabil*, 86 (1), 162-166.

**Author Information**

**MS Wong**

Department of Health Technology and Informatics, The Hong Kong Polytechnic University

**D Wong**

Department of Health Technology and Informatics, The Hong Kong Polytechnic University

**A Wong**

Department of Health Technology and Informatics, The Hong Kong Polytechnic University